


Sensor Application

TEMPLE TOUCH PRO™
Non-Invasive Core Temperature System

1

Wipe Temple Area Clean


- » Use alcohol wipe
- » Allow to dry or wipe dry with gauze

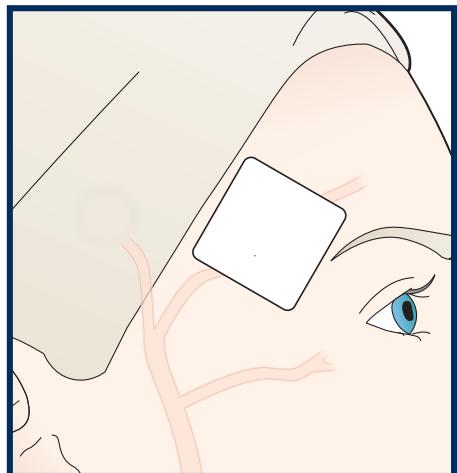

2

Remove Adhesive Backing & Apply Sensor over Temporal Artery


- » Place sensor on temporal artery
- » Avoid placing sensor on "soft spot", hairline, or sinuses
- » Gently press for 2-3 seconds
- » For **ENT procedures**, place sensor on non-operative side
- » For **BIS™ monitoring**, apply TTP sensor prior to applying BIS sensor

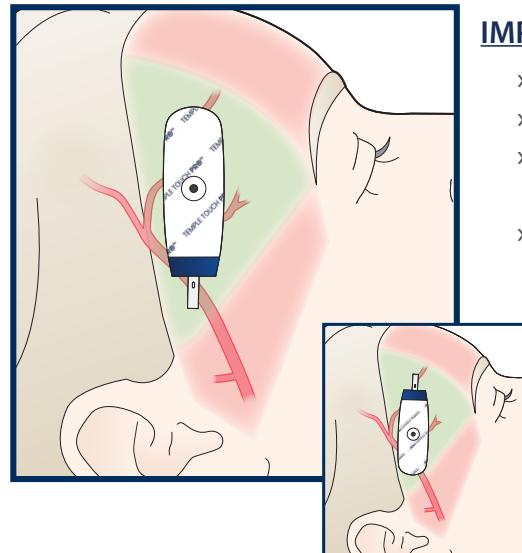

3

Connect Sensor to Sensor Connecting Unit (SCU)

- » Hold close to connection points when connecting
- » Carefully insert the sensor tab
- » Confirm blue stripes align

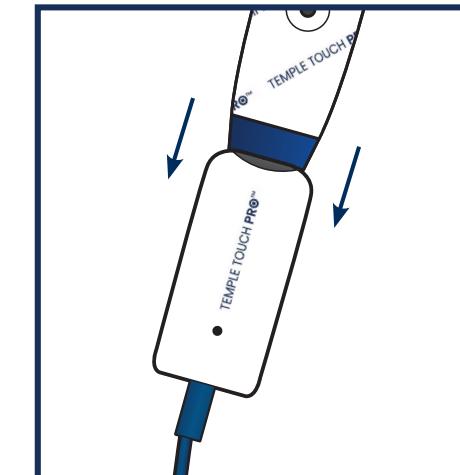

4

Attach SCU Securement Clip

- » Prevents unintended drag/pull on sensor
- » Use gown, bouffant cap, pillow, sheet, etc.

